
Infrared thermometer Instruction manual

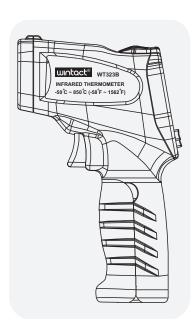


Version: WT323B-EN-00

-1-

2. Locating a Hot Spot:

To find a hot spot, aim the thermometer outside of interest, then scan across with an up and down motion until you locate the hot spot. (Figure 2).




d

е


F. LCD display & buttons

- LCD: as shown in Figure 3.
- a. Temperature reading b. Temperature units
- c. Low battery indicator d. Turning on state indicator of positioning
- laser
- e. K-type thermocouple f. Data reading indicator g. Data holding indicator h. Mode display
- Trigger locking indicator j. Trigger unlocking
- cator k. Low temperature alarm I. High temperature alarm



A DATA D

h



(1) Measurement switch (trigger).
Pull trigger to display temperature value, and
"SCAN" appears on screen at the same time; when
trigger is released, temperature reading is displayed,
and data is automatically maintained. The instrument
is automatically turned off after about 30 seconds of
operation.

A.Introduction

This infrared thermometer is used for measuring the temperature of the object's surface, which is applicable for various hot, hazardous or hard-toreach objects

without contact safely and quickly.

This unit consist of Optics, Temperature Sensor Signal amplifier, Processing circuit and LCD Display.

The Optics collected the infrared energy emitted by object and focus onto the Sensor. Then the sensor translates the energy into an electricity signal. This signal will be turned out to be digital shown on the LCD after the signal amplifier and processing circuit.

B. WARNING & CAUTIONS

1. Warning:
To avoid the potential situation may cause harm or damage to people, please pay attention to the following items:

- 1). Do not point laser directly at eye or indirectly off
- reflective surfaces.
 2). The unit cannot measure through transparent surfaces such as glass or plastic. It will measure the surface temperature of these materials instead.
- Steam, dust, smoke, or other particles can prevent accurate measurement by obstructing by the units optics.


2. Cautions:
Infrared thermometer should be protected for the following:

1). EMF (electro-magnetic fields) from arc welders,

- induction heaters.
- Thermal shock (cause by large or abrupt ambient temperature changes allow 30 minutes for unit to stabilize before use).

 Do not leave the unit on or near objects of high
- temperature.

C. Distance to spot size



-2-

(2) Laser switch/Down button.
(3) MODE (mode switch button) / temperature unit switch button.
Press MODE button to cycle through the following

modes, MAX→MIN→dIF→HAL→LAL→EMS→LOG→
K-T.The instrument memorizes the current measurement mode, the next time the mode will be that of last time after startup.
a.MAX: Maximum value of the last measured data.

b.MIN: Minimum value of the last measured data. **c.dIF:** Difference between maximum and minimum

c.dIF: Difference between maximum and minimum value.

d.HAL (High temperature alarm):
When HAL is selected, press up/down button to set high temperature alarm point. When the measured temperature is higher than setting point, high temperature alarm indicator appears and sound of "bi bi..." goes off.

e.LAL (Low temperature alarm):
When LAL is selected, press up/down button to set high temperature alarm point. When the measured temperature is lower than setting point, low temperature alarm indicator appears and sound of "bi bi..." goes off.

f.EMS (Emissivity):
When EMS is selected, press up/down button to set value within 0.10 to 1.00.
g.LOG (Storage function):
After each measurement, the measured data is automatically recorded (LOG); a total of 100 groups can be recorded, the first group will be automatically covered if more than 100 groups, and so on. When LOG is selected, press up/down key to review the data measured before.
h.K-T(K-type thermocouple temperature measurement mode):
Under this mode, the temperature of the K-type thermocouple is measured and thermocouple icon is displayed. Before the measurement, insert K-type thermocouple probe into thermocouple socket. Pull and hold trigger, thermometer displays both surface temperature units switch:
Pull and hold trigger then press temperature units switch button to switch units.

(4) UV light button / trigger locking button / Up button.
a. UV light:

1. When take measurement, pay attention to the Distance to Spot Size. As the Distance (D) from the target surface increases, the spot size (S) of the area measured by theunit becomes larger.

The Distance to Spot size of the unit is 12:1.(Figure 1)

Field of view:

Make sure the target is larger than the unit's spot size. The smaller the target the closer measure distance. When accuracy is critical, make sure the target is at least twice as large as the spot size.

Emissivity: Most organic materials and painted or oxidized surfaces have an emissivity of 0.95(preset in the unit). Inaccurate readings will result from measuring shiny or polished metal surfaces. To compensate for this, adjust the units emissivity reading or cover the surface to be measured with

masking tape or flat black paint.

Measure the tape or painted surface when the tape or painted reach the same temperature as the material underneath.

Marterial Emissivity Marterial Emissivity Aluminum 0.30 Iron 0.70 Asbestos 0.95 Lead 0.50 Asphalt 0.95 Limestone 0.98 0.70 0.94 Basalt Oil Brass 0.50 Paint 0.93 0.90 Paper 0.95 Brick Plastic Carbon 0.85 0.95 0.95 Rubber 0.95 Ceramic Concrete 0.95 Sand 0.90 Copper 0.95 Skin 0.98 Dirt 0.94 Snow 0.90 0.90 Steel 0.80 Frozen food Hot food 0.93 Textiles 0.94 Glass(plate) 0.85 Water 0.93

Ice E. Operation

Wood

0.94

0.98

Operating the unit:
Open battery door and load two 1.5V AAA batteries.
Pull the trigger to turn on the unit.
Aim at the target surface and pull the trigger, then temperature will be shown on the LCD. This unit is equipped with a laser, which is only used for aiming

-3-

(5) Battery door

UV light

Infrared temperature sensing area

Laser (assisted positioning)

K-type thermocouple socket

G. Maintenence

Lens Cleaning:
Blow off loose particles using clean compressed air.
Gently brush remaining debris away with a moist cotton swab. The swab may be moistened with water.

2. Case cleaning:

Clean the case with a damp sponge/cloth and mild soap.

1) Do not use solvent to clean plastic lens.

2) Do not submerge the unit in water.

H. Specification

LCD	Colorful LCD
Temperature measurement range	−50 °C~ 850°C (−58°F ~ 1562°F)
Temperature display accuracy	0.1°C
Temperature measurement error	-50°C~0°C(-58°F~32°F):±3°C (±5°F) 0°C~850°C(32°F~1562°F):±1.5% rdg or±1.5°C (±2.7°F) Take the bigger value
Repeatability	1% rdg or 1°CTake the bigger value
Reponse time	0. 5s, 95% Response
Emissivity	0.10~1.00 Adjustable(preset as 0.95)
D:S	12:1
Response wavelength	8um~14 um
Laser	Ring light spot
Flashlight	UV light
Working environment temperature	0 °C~40°C (32°F ~ 104°F)
Relative working environment humidity	10% RH~90% RH withput condensation
Storage temperature	-10 °C~ 60°C (14°F~140°F)
Batteries	1. 5V AAAbattery*2(No.7 battery)
Low power indicator	Low power indicator for power below 2.4V
Overload indicator	"Hi"/"Lo" displayed on LCD
Weight/dimensions	202g(including batteries) /108*49*177 mm

Specifications of K-type thermocouple

Measurement range 0°C~250°C (300°C for short time)

Measurement error ±2.5°C or 0.75% rdg Take the bigger value Thermal response time < 10s

Specific Declarations: Our company shall hold no any responsibility resulting from using output from this product as an direct or indirect evidence. We reserves the right to modify product design and specification without notice. -6-



