CM4371-50 CM4373-50 CM4375-50




# **Instruction Manual**



ΕN



# AC/DC CLAMP METER



Mar. 2023 Revised edition 1 CM4371C961-01

# **Contents**

Intro	oducti	on	1
		Package Contents	
		ormation	
		Precautions	
1	Ov	erview	19
	1.1 1.2	Product Overview and Features Part Names	
2	Ма	king Measurements	21
	2.1	Inspection Before Measurement	21
	2.2	Installing Batteries and the Z3210 Wireless Adapter	
		Installation procedure	
	2.3	Use of Test Leads	27
		L9300 Test Lead (accessory)	29

#### Contents

2.4	Current Measurement	32
	Manual hold, automatic hold	34
	Switching the ranges	
	Filter function	
	Maximum value, minimum value, average, and peak value	40
	Inrush current (inrush)	
2.5	Various Other Measurement Functions	
2.6	LCD Backlight, Automatic Power Save (APS)	
2.7	DC High V Probe Mode	
2.8	Wireless communications function	
	Using GENNECT Cross	
	Z3210-to-Excel <sup>®</sup> direct data entry function	
	(Excel® direct input function, HID function)	55
2.9	Rotary Switch Combinations	
C to	a aifi a ati a na	C4
Sp	ecifications	61
3.1	General Specifications	61
3.2	Input Specifications, Measurement Specifications	
3.3	Accuracy table	
J.J	ACCUIACY LADIC	/

4_	Maintenance and Service	
	4.1 Troubleshooting	109
5	Appendix	
	5.1 Voltage Detection Function	111 113
Ind	lex	115
Wa	rranty Certificate	119

#### Contents

## Introduction

Thank you for choosing the Hioki CM4371-50/CM4373-50/CM4375-50 AC/DC Clamp Meter. To ensure your ability to get the most out of this instrument over the long term, please read this manual carefully and keep it available for future reference.

Read the separate document "Operating Precautions" carefully before using the instrument.

#### Latest edition of instruction manual

The contents of this manual are subject to change, for example as a result of product improvements or changes to specifications.

The latest edition as well as multilingual editions of the manual (in Chinese, French, German, Italian Korean, and Spanish) can be downloaded from Hioki's website.



https://www.hioki.com/global/support/download

#### **Product registration**

Register your product in order to receive important product information. https://www.hioki.com/global/support/myhioki/registration



#### Introduction

### **Target audience**

This manual has been written for use by individuals who use the product in question or who teach others to do so. It is assumed that the reader possesses basic electrical knowledge (equivalent to that of someone who graduated from the electrical program at a technical high school).

#### **Trademarks**

- Microsoft Excel is a registered trademark or a trademark of Microsoft Corporation in the United States and other countries.
- The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Hioki E.E. Corporation is under license. Other trademarks and trade names are those of their respective owners.

# Notations

### Safety notations

In this document, the severity levels of risk and hazard are classified as follows.

<b>▲</b> DANGER	Indicates an imminently hazardous situation that, if not avoided, will result in death or serious injury.	0	Indicates an action that must not be performed.
<b>≜WARNING</b>	Indicates a potentially hazardous situation that, if not avoided, could result in death or serious injury.	•	Indicates an action that must be performed.
<b> △ CAUTION</b>	Indicates a potentially hazardous situation that, if not avoided, could result in minor or moderate injury or potential risks of damage to the supported product (or to other property).	A	Indicates a high-voltage hazard. Failure to verify safety or improper handling of the instrument could lead to electric shock, burn injury, or death.
IMPORTANT	Indicates information or content that is particularly important from the stand point of operating or maintaining the instrument.		Indicates the presence of a hazard caused by a strong magnet. The product could interfere with the proper operation of electronic medical devices such as pacemakers.

#### **Notations**

## Symbols shown on the instrument

$\triangle$	Indicates the presence of a potential hazard. For more information about locations where this symbol appears on instrument components, see the "Operating Precautions" (p. 12) and the accompanying document entitled "Operating Precautions."
A	Indicates that a dangerous voltage is generated from this terminal.
4	Indicates that the product can be attached or detached while the circuit is live.
	Indicates the instrument is protected throughout by double insulation or reinforced insulation.
$\sim$	Indicates alternating current (AC).
===	Indicates direct current (DC).
=	Indicates the grounding terminal.

## Symbols for various standards



Indicates that the product is subject to the Waste Electrical and Electronic Equipment (WEEE) Directive in EU member nations.



Indicates that the product complies with standards imposed by EU directives.

## Screen display

The instrument screen displays the alphanumeric characters as follows.



Exception

**OPEn**: Wire break detected



#### **Notations**

## **Accuracy labeling**

Instrument accuracy is expressed by defining a percentage of the reading, a percentage of full scale, a percentage of the setting, or a limit value for errors in terms of digits.

Reading (display value)	Indicates the value displayed by the instrument.  Limit values for reading errors are expressed as a percentage of the reading ("% rdg").
Full scale (maximum display value)	Indicates the maximum display value for each measurement range. Measurement range values for the instrument indicates that maximum display value. Limit values for full-scale errors are expressed as a percentage of full scale ("% f.s.").

#### Other notations

(p. ) Indicates the page number to reference.		
* Indicates additional information is described below.		
CM4371.50 Indicates that the item is applicable to the CM4371-50 only.		

# **Checking Package Contents**

When you receive the instrument, inspect it to ensure that no damage occurred during shipment. Pay particular attention to included accessories, panel keys, and terminals. If you find any damage or discover that the instrument does not perform as indicated in its specifications, please contact your authorized Hioki distributor or reseller.





# **Options**

The options listed below are available for the instrument. To order an option, please contact your authorized Hioki distributor or reseller.

Options are subject to change. Check Hioki's website for the latest information.

#### **Connection cables**

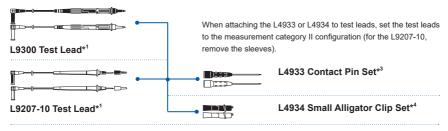

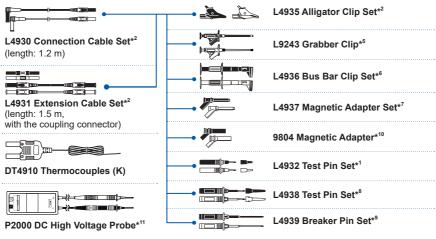

- \*1: CAT IV 600 V, CAT III 1000 V, CAT II 1000 V, 10 A
- \*2: CAT IV 600 V, CAT III 1000 V, 10 A
- \*3: 30 V AC, 60 V DC, 3 A
- \*4: CAT III 300 V, CAT II 600 V, 3 A
- \*5: CAT II 1000 V, 1 A
- \*6: CAT III 600 V, 5 A

- \*7: CAT III 1000 V, 2 A
- \*8: CAT III 600 V, CAT II 600 V, 10 A
- \*9: CAT III 600 V, 10 A
- \*10: CAT IV 1000 V, 2 A
- \*11: CAT IV 1000 V, CAT III 2000 V

#### Options

### **Carrying cases**

The instrument, test leads, and the instruction manuals can be accommodated.

#### C0203 Carrying Case



C0207 Carrying Case



### **Z3210 Wireless Adapter**




Connecting the Z3210 to the instrument enables the wireless communication function.

See "2.8 Wireless communications function" (p.51).

# **Safety Information**

### Measurement categories

The instrument conforms to the safety requirements for CAT III 1000 V and CAT IV 600 V measuring instruments.

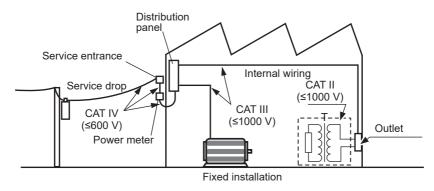

# **Operating Precautions**

Observe the following precautionary information to ensure that the instrument can be used safely and in a manner that allows it to perform as described in its specifications. Carefully read the separate document entitled "Operating Precautions" before use. Use of the instrument should conform not only to its specifications, but also to the specifications of all accessories, options, and other equipment in use.

## **A** DANGER

■ Do not touch the section beyond the barrier during operation.

Failure to do so could cause the operator to experience an electric shock. See "1.2 Part Names" (p.20).

■ Do not measure any current in excess of the derating curve.



Doing so can cause overheating of the sensor, resulting in bodily injury, fire, or damage to the instrument.

See "Frequency derating characteristics" (p.68).

The maximum measurement current varies with the frequency, and the current that can be measured continuously is limited. Operating the instrument at less than this limitation is referred to as derating.

## **A DANGER**

■Inspect the instrument and verify proper operation before use.



Use of the instrument while malfunctioning could result in serious bodily injury. If you find any damage, contact your authorized Hioki distributor or reseller. See "2.1 Inspection Before Measurement" (p.21).

■ Confirm that the white portion (insulation layer) inside the cable is not exposed.

Using the instrument with a color inside its cable exposed could cause the operator to experience an electric shock.

## **MARNING**

- Do not allow the instrument to get wet.
- Do not take measurements with wet hands.

Failure to do so could cause the operator to experience an electric shock.



■When using the instrument while connected to test leads, do not make measurements that exceed either of the ratings indicated on the instrument or on the test leads, whichever is lower.

Using the instrument to make measurements that exceed either rating could cause the operator to experience an electric shock.

#### **IMPORTANT**



- Do not allow any foreign object to be caught between the facing core surfaces of the jaws.
- Do not scratch the facing core surfaces of the jaws.



- Do not touch the facing core surfaces of the jaws with your fingers.
- Do not insert any foreign object into the gap of the jaws.



- Do not drop the instrument.
- Do not subject the instrument to any shock.

Doing so may adversely affect the measurement accuracy and open/close operation.

Clamp the instrument around only one conductor. Clamping the instrument around two or more of conductors in a bundle prevents the instrument from measuring any current regardless of whether the measurement target is a single-phase or three-phase circuit.

L4937 Magnetic Adapter Set / 9804 Magnetic Adapter (optional)

## **A** DANGER

■ People with electronic medical devices such as pacemakers should not use the magnetic adapter.



■ Keep the magnetic adapter away from the body.

Failure to do so may affect proper operation of the electric medical devices, presenting a hazard to human life.

## **ACAUTION**

- Do not drop the magnetic adapter.
- Do not subject the magnetic adapter to mechanical shock.

Doing so could damage the magnetic adapter.

■ Do not use the magnetic adapter in locations where it may be exposed to rainwater, dust, or condensation.



Doing so could decompose or deteriorate the magnetic adapter. In addition, diminished magnetic adhesion cause the instrument to drop, resulting in damage to the instrument.

- Do not bring the magnetic adapter near magnetic storage devices, such as floppy disks, magnetic cards, prepaid cards, or magnetized tickets.
- Do not bring the magnetic adapter near precision electronic equipment, such as computers, TV screens, or electronic wrist watches.

Doing so could damage such devices or data stored in them.

Operating Precautions

# **Overview**


## 1.1 Product Overview and Features

This instrument is a clamp meter that can perform true RMS measurement of current simply by clamping it around a circuit. In addition to current, it can measure voltage, frequency, rush current, resistance, diode, capacitance, temperature, and AC power. Installing the Z3210 Wireless Adapter (optional) to the instrument allows your mobile device to display waveforms and measure harmonics.

#### Measurement function list

A+V VA	DC current and DC voltage, DC power
NCV	Electric charge detection  CM4371 <sub>-50</sub> CM4373 <sub>-50</sub>
TEMP	Capacitance, temperature
<b>→</b> Ω →	Continuity check, resistance, diode
$_{ m AUTO}^{==\cdot}$ V	Automatic AC/DC, AC voltage, DC voltage, AC+DC voltage, frequency
$\overset{=}{AUTO} \mathbf{A}$	Automatic AC/DC, AC current, DC current, AC+DC current, frequency

## 1.2 Part Names



- 1 Operation grip
- **2** Fn key (allows you to choose a function)
- 3 Jaws
- 4 Barrier
- 5 Serial number (The serial number consists of 9 digits. The first two (from the left) indicate the year of manufacture, and the next two indicate the month of manufacture.)
- 6 Rotary switch See "Measurement function list" (p. 19).
- 7 HOLD key
- 8 LCD
- 9 Battery cover
- 10 Operation keys
- 11 Measurement terminals
- 12 Strap hole

# **Making Measurements**

# 2.1 Inspection Before Measurement

Check	Inspection details	Check	Inspection details
	The battery cover is closed and its screw has been securely tightened.		There is no damage to the test lead insulation, and neither the white sheathing nor metal conductor inside the wire are exposed.
	There is no foreign matter on the measurement terminals (p. 20).		The instrument is neither damaged nor cracked.
	The test leads are not broken (p.43).		No segments are missing.    Constitution   Constitu
	OK (1 Ω or less)		(All segments appear)

# 2.2 Installing Batteries and the Z3210 Wireless Adapter

Installing the Z3210 to the instrument enables the wireless communications function. (p.51)

# **MARNING**

■ Before removing the battery cover, remove the instrument from an object under measurement and set the rotary switch to the OFF position.



Failure to do so could cause the operator to experience an electric shock. When the instrument is clamped around the object under measurement, the battery contact terminals are regarded as high-voltage parts.

## **MARNING**

■ After replacing the batteries or installing/removing the Z3210 Wireless Adapter, install the battery cover and tighten the screw, then use the instrument.



Use of the instrument with the battery cover removed could result in bodily injury.

■ Secure the battery cover with the screw attached to the instrument at the time of shipment.

If you have lost the screw or find that the screw is damaged, please contact your authorized Hioki distributor or reseller.

## **A CAUTION**

- Do not mix batteries of different ages or types.
- Do not use a battery whose recommended service life has expired.



- Do not reverse the battery polarity.
- Do not leave the exhausted batteries in the instrument.

Doing so may cause the batteries to leak, damaging the instrument.

- Use the specified type of batteries only (LR03 Alkaline batteries).
- Remove the batteries when the instrument is not in use for an extended period of time.



Doing so may cause the batteries to leak, damaging the instrument.


■ Before handling the Z3210, eliminate static electricity on your body by touching any metallic part, such as a doorknob.

Failure to do so may cause static electricity to damage the Z3210.

- When the I mark blinks, the batteries will be exhausted. Replace the batteries with new
  ones in good time. The instrument may be turned off when the display is backlighted or the
  buzzer sounds. After use, be sure to turn off the instrument.
- Dispose of the batteries in accordance with local regulations.

### Installation procedure

Read the precautions before performing the procedure. (p.22)

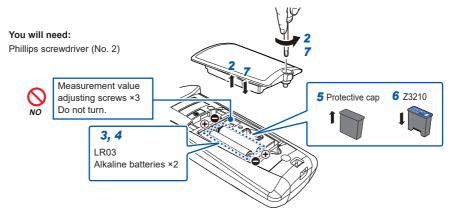

0

Do not turn any screws except the battery cover screw.

After removing the battery cover, you will find three screws, which are used to adjust measured values. Do not turn them because the instrument will not be able to perform measurement accurately.

#### Installing Batteries and the Z3210 Wireless Adapter

- 1 Remove the instrument from an object under measurement and set the rotary switch to the OFF position.
- 2 Loosen the screw and remove the battery cover.
- 3 Remove the old batteries (when replacing the batteries).
- Install fresh batteries, observing the correct polarity.
  When installing the Z3210 Wireless Adapter, go on to step 5.
  When not installing the Z3210 Wireless Adapter, go on to step 7.
- 5 Remove the protective cap from the instrument.
- 6 Install the Z3210 Wireless Adapter, observing the correct orientation.
- 7 Reattach the battery cover and tighten the screw.

## 2.3 Use of Test Leads

The L9300 Test Lead (accessory) or the L9207-10 Test Lead (optional) is used for measurement. Depending on measurement locations, use Hioki's optional measurement cables. See "Options" (p.8)

# **MARNING**



■ When using the instrument, use the test leads and options specified by Hioki.

Using test leads and options other than those specified could cause bodily injury or short circuit accidents.

- When measuring the power line voltage, use test leads that satisfy the following conditions.
  - IEC 61010 or EN 61010 safety standard-compliant



- · Rated for measurement category III or IV
- · With the rated voltage higher than voltage being measured

Failure to do so could cause the operator to experience an electric shock.

The optional test leads for this instrument comply with the EN 61010 safety standard. Observe the measurement category and rated voltage indicated on the test leads during use.

## **A** CAUTION



Do not bend the cables at temperatures of 0°C or lower. Do not pull on the cables.

The cables can become rigid. Doing so could damage the insulation or cause a wire break, resulting in an electric shock.

## L9300 Test Lead (accessory)

See the precautions in "Use of Test Leads" (p. 27) as well.

## **WARNING**

Use the test leads with the correct measurement category displayed.




■ Do not use the test leads if the metal pin is bent or the protective finger guard does not slide properly.

Doing so could cause short circuit accidents.


### Switching the measurement category

#### 1 Unlock the protective finger guard.


Rotate the grip to unlock, moving the  $\triangleright$  mark along the guide line.



### 2 Slide the protective finger guard.



#### 3 Lock the protective finger guard.



Perform the above steps to switch over from measurement category III to measurement category III or IV as well.

## 2.4 Current Measurement

1 Rotate the rotary switch.




2 Hold down for 1 s.



#### **IMPORTANT**

Always perform zero adjustment to perform accurate measurement.

3 Clamp the instrument around the wire.



#### Frequency detection range for AC current


CM4371-50	20.00 A range	4.00 A or more
GIVI437 1-30	600.0 A range	20.0 A or more
ON44070 FO	600.0 A range	40.0 A or more
CM4373-50	2000 A range	200 A or more
CM4375-50	_	5.0 A or more

#### DC voltage polarity check (p.59)

If the measured value is negative, the buzzer will sound and the display will be backlighted in red. (threshold: -10 A)

## Manual hold, automatic hold


#### Manual hold



HOLD The measured value freezes. ►

Press the **HOLD** key again to disable the hold function.

## Automatic hold



The measured value freezes automatically.


Holding down the **HOLD** key for 1 s to disable the automatic hold function.

#### **Automatic hold conditions**

Displayed value will freeze when the following two conditions are satisfied at the same time:

- When the measured value fluctuation stabilizes within the fluctuation range described in the table on the next page.
- When the measured value exceeds the threshold value described in the table on the next page (voltage, current).

When the measured value is less than the threshold value described in the table on the next page (resistance, continuity check, diode).

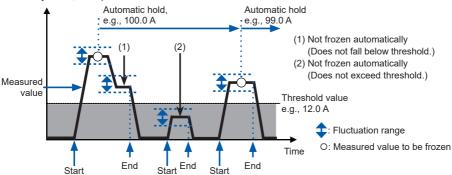

Suppose that the measured value has fallen below (voltage, current) or exceeded the threshold value (resistance, continuity, diode) after the displayed value froze. When the two auto-hold conditions are met again after that, refreshing measured values will stop.

#### **Current Measurement**

Measurement function* <sup>1</sup>	Measurement range	Fluctuation range	Threshold value
Auto A AC current DC current	20.00 A range (CM4371-50)	Within 1.00 A	1.00 A
AC+DC current	600.0 A range (CM4371-50, CM4373-50)	Within 12.0 A	12.0 A
	1000 A range (CM4375-50)	Within 12.0 A (When inputting more than 12.0 A) Within 1.0 A (When inputting more than 12.0 A)	12.0 A (When inputting more than 12.0 A) 0.9 A (When inputting more than 12.0 A)
	2000 A range (CM4373-50)	Within 40 A	40 A


Measurement function*1	Measurement range	Fluctuation range	Threshold value
Auto V* <sup>2</sup> AC voltage DC voltage* <sup>2</sup> AC+DC voltage	6.000 V, 60.00 V, 600.0 V range	Within 120 counts	120 counts
ACTDC Vollage	1000 V range	Within 20 V	20 V
DC High V Probe Mode	600.0 V range	Within 12.0 V	80.0 V
	2000 V range	Within 20 V	80 V
Continuity check Resistance	$600.0~\Omega$ range, $6.000~\kappa\Omega$ range, $60.00~\kappa\Omega$ range, $60.00~\kappa\Omega$ range, $600.0~\kappa\Omega$ range, $6.000~\kappa\Omega$ range	Within 100 counts	4900 counts
Diode	1.800 V range	Within 0.040 V	1.460 V

<sup>\*1:</sup> The automatic hold function does not support measurement functions not listed in this row.

<sup>\*2:</sup> Except the 600.0 mV range (only when the range is set manually)


## Switching the ranges

#### When the CM4373-50 measures current

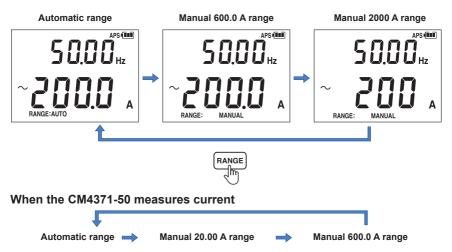


The CM4375-50 provides the 1000 A range only.

#### Filter function

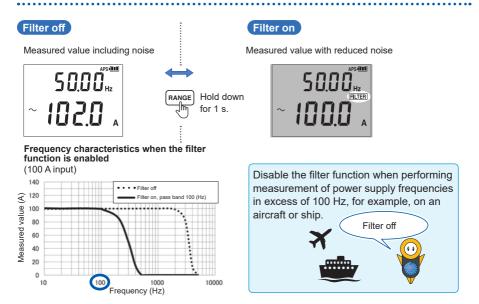

## Maximum value, minimum value, average, and peak value

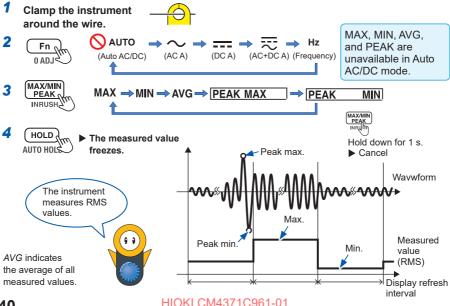


## Inrush current (inrush)

- 1 Turn off the motor.
- 2 Rotate the rotary switch.



3 Hold down for 1 s.




4 Clamp the instrument around the wire.

See "Inrush trigger level" (p.67).



5 Set the range.




In automatic ranging mode, the instrument will be automatically set to the 600.0 A range (CM4371-50), 2000 A range (CM4373-50).

6 Hold down for 1 s.




7 Turn the motor on.






(Inrush current occurs)









Inrush current occurrence period (about 10 ms to 999 ms)

## 2.5 Various Other Measurement Functions


#### **Voltage measurement**







#### DC voltage polarity check (p.59)

If the measured value is negative, the buzzer will sound and the display will be backlighted in red. (threshold: -10 V)

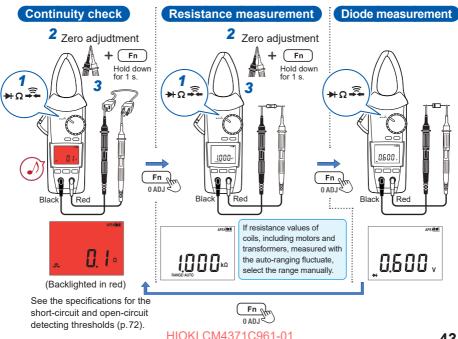

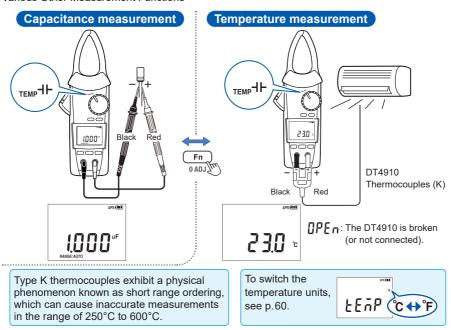

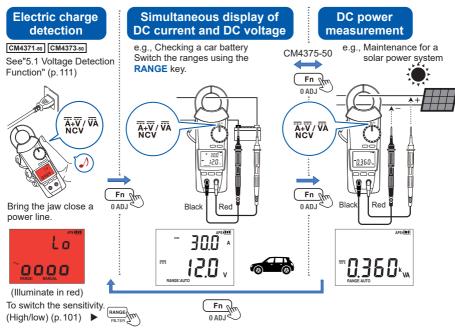

## 2.6 LCD Backlight, Automatic Power Save (APS)


#### LCD backlight



Backlight off



Backlight on Automatically shut off after 40 s of inactivity



The instrument is automatically turned off. Set the rotary switch to the OFF position to restart.

# 2.7 DC High V Probe Mode

Use of the P2000 DC High Voltage Probe (optional) allows you to measure DC voltage of up to 2000 V (CAT III 2000 V, CAT IV 1000 V), such as open voltage of solar panels.

## **MARNING**

■ Do not use the P2000 to measure AC voltage.



The probe cannot accurately measure AC voltage. Improper measurement could lead to electric shock. You can use the P2000 for DC voltage measurement only.

■ Do not measure voltage that exceeds 2000 V DC.

Doing so could damage the instrument and the P2000, causing bodily injury.



■ Use the P2000 to measure voltage that exceeds 1000 V.

Use of other probes could cause the operator to experience an electric shock.

## **ACAUTION**



■ Connect the instrument and the P2000 together with the strap when using the L4943.


The cables and plugs will be subjected to stress, damaging them.

#### When using the L4943 Connection Cable Set\*


Disconnect the clip\* from the strap buckle\* as shown in the figure.



2 Attach the strap\* to the P2000. For details, see the P2000 Instructon manual.



3 Attach the strap buckle to the instrument and connect it to the clip that you attached to the P2000 with the strap.



\*: Supplied with the P2000.

When using the L4930 Connection Cable Set or the L4931 Extension Cable Set (optional)

Hang the P2000 in some way, such as using a magnetic strap, not to subject the cables and the plugs to stress.

#### **Making Measurements**

Rotate the rotary switch.




Hold down the two keys for 1 s as described below.




▶ DC High V Probe mode On







- Connect the P2000 DC High Voltage Probe to the measurement terminals of the instrument.
- Set the range.



Bring the probes into contact with an object to be measured

49

#### DC High V Probe Mode

#### Saving the DC High V Probe mode settings

Turn off the instrument, and then set the rotary switch to other than the OFF position while holding down the two operation keys as described below.



- The DC High V Probe mode start-up setting can be toggled between on and off. (p.59)
- When the DC High V Probe mode start-up is enabled, the instrument will start in the mode you last used.

## 2.8 Wireless communications function

Installing the Z3210 Wireless Adapter (optional) is required. Concurrent use of GENNECT Cross and HID function (p.55) is not available.

## **Using GENNECT Cross**

Enabling the wireless communications function allows you to check and record the measured data of the instrument, and create measurement reports using your mobile device. For details, see the operation guide for the GENNECT Cross app (free of charge).

#### **GENNECT Cross special site**

https://gennect.net/en/cross/index



#### Using the wireless communications function

- Connect the Z3210 Wireless Adapter (option) into the instrument. (p.22)
- Install GENNECT Cross on your mobile device.
- 3 Turn on the instrument.
- 4 Enable the wireless communications function.

When the instrument is turned on for the first time after the Z3210 has been installed, the wireless communications function will be enabled.



Hold down for 1 s.

## n) appears:

# Wireless communications function enabled

Off: Wireless communications function disabled Blinks: During wireless communications

### 5 Start GENNECT Cross and register the connection of the instrument.

- When GENNECT Cross is started for the first time (when there is no registered instrument), the Instrument Settings screen appears.
- When the instrument is placed near your mobile device, its connection is registered automatically on the Instrument Settings screen of GENNECT Cross (up to eight instruments).
- Wait for 5 to 30 s until the connection of the instrument is registered after turning on the instrument. If the connection of the instrument is not registered after 1 minute has elapsed, restart GENNECT Cross and the instrument.
- Select a measurement function to perform measurement.

- The communication distance is about 10 m with a clear line of sight. The communicable
  distance may vary greatly depending on the presence of an obstruction (wall or metallic
  shielding object) and the distance between the floor (ground) and instrument. To ensure the
  stable communication, make sure that the radio wave intensity is sufficient.
- GENNECT Cross is free of charge. However, the customer is responsible for the cost to download the application software and connect to the Internet when using the software.
- GENNECT Cross may not operate properly depending on the mobile device.
- The Z3210 uses the 2.4 GHz band wireless technology.
   When there is a device that uses the same frequency band such as a wireless LAN (IEEE 802.11.b/g/n) near your mobile device, the communication may not be established.

When the instrument is placed on the floor or ground, the communication distance becomes shorter. It is recommended that you move the instrument away from the floor or ground and place it on a desk or table or hold it by hand.

#### Wireless communications function

#### **Event recording function**

The event recording function logs the data when a measured value exceeds a desired threshold value, which can be set with GENNECT Cross. For details, see the operation guide for the GENNECT Cross app (free of charge). The number of recorded events can be checked using the instrument



- Up to 99 events can be recorded. If events has reached 99, the event recording will stops.
   When another event recording starts, previously recorded data will be deleted.
- Some events with a duration time of less than 400 ms may not be accurately measured, failing to detect them.\*
  - \* Current frequency, voltage frequency, capacitance (400 ms to 4000 ms, depending on measured value), temperature (type K thermocouple) 2000 ms

# Z3210-to-Excel<sup>®</sup> direct data entry function (Excel<sup>®</sup> direct input function, HID function)

Concurrent use of GENNECT Cross and HID function is not available.

The human interface device (HID) profile, with which the Z3210 Wireless Adapter is equipped, is a profile same as that wireless keyboards use.

HID ON	Preparatory to data entry, open an Excel <sup>®</sup> file on your mobile device or computer and choose a cell. When the instrument's display freezes, the measured values will be entered on the cells. The use of this function with the automatic hold function enabled comes in handy. (p.34)
HID OFF	When you wish to use GENNECT Cross, disable the HID function.

The setting whether the HID function has been enabled or disabled will not be saved in the instrument but in the Z3210.



#### Confirming the HID setting

- 1 Remove the test leads from the object under measurement.
- Set the rotary switch to the OFF position.
- 3 Connect the Z3210 Wireless Adapter (option) into the instrument. (p.22)
- 4 Confirm the HID setting.

Make sure that the instrument is turned off, and then set the rotary switch to the TEMP position while holding down the RANGE key.



The settings stored in the Z3210 will be displayed.



au H 'q

or


#### When [- - - - ] appears

Update the Z3210 firmware to the latest version using GENNECT Cross (version 1.8 or later)...


To change the HID setting, use the procedure on the following page.

#### Changing the HID setting

- 1 Turn off the instrument.
- 2 Chang the HID setting.



After exhibiting the following displays, the instrument is automatically turned off.

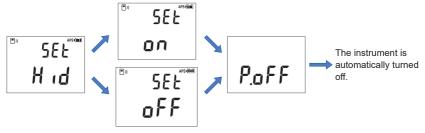

3 Turn on the instrument again.

The HID setting will be toggled.

#### **IMPORTANT**

#### To switch over from the HID function to GENNECT Cross

If you start GENNECT Cross without canceling the paring between the mobile device and the instrument, GENNECT Cross may not be able to recognize the instrument as a connectible device. Follow the procedure below to reconnect the instrument to GENNECT Cross. Use the **Bluetooth**® setting of your mobile device to delete the instrument.

- 1. Disable the Z3210's HID function. (p.57)
- 2. Use the Instrument Setting of GENNECT Cross to reconnect the instrument.

Check Hioki's website for the latest information.

https://z3210.gennect.net



Learn more here!

# 2.9 Rotary Switch Combinations



# Turn off the instrument, and then turn it on again while holding down one or two operation keys.

(Set the rotary switch to other than the OFF position)

Setting	Procedure	Factory- shipped setting	Saving of setting
Auto-power save (APS) function cancel	HOLD + Any position	On	Not saved
DC current/voltage, polarity check on/off	Fn + Any position	Off	Saved
LCD all segments display* <sup>1</sup> , firmware version number* <sup>1</sup> , model number (only last four digit)* <sup>1</sup> , serial number* <sup>1</sup> , HID setting check (Z3210 required)* <sup>1</sup>	RANGE + ( Any position	-	-
Buzzer (on/off)	MAX/MIN + Any position	On	Saved
Automatic backlight shutoff (on/ off)	Any position	On	Saved
DC High V Probe mode setting saving (on/off)	Any position	Off	Saved

#### **Rotary Switch Combinations**

Setting	Procedure	Factory- shipped setting	Saving of setting
Toggling the HID setting (on/off) (Z3210 required)		-	-* <sup>2</sup>
Switching between the two temperature units: degrees Celsius and degrees Fahrenheit	Fn + HOLD + MAX/MIN + RANGE Hold down for 1 s.  To switch the temperature units  To save the setting MAX/MIN PEAK Hold down for 1 s.	Degrees Celsius	Saved

<sup>\*1:</sup> The screen display depends on the rotary switch position.

<sup>\*2:</sup> The setting whether the HID function has been enabled or disabled will not be saved in the instrument but in the Z3210.

3

# **Specifications**

# 3.1 General Specifications

Operating environment	Indoor use, pollution degree 2, altitude up to 2000 m (6562 ft.)
Operating temperature and humidity range	-25°C to 65°C (-13°F to 149°F), 90% RH or less (non-condensing)
Storage temperature and humidity range	−30°C to 70°C (−22°F to 158°F), 90% RH or less (non-condensing, with batteries removed)

### **General Specifications**

Dust resistance and water resistance	<ul> <li>IP20 (When measuring voltage under completely dry conditions, when measuring current flowing through a hazardous live conductor under completely dry conditions)</li> <li>IP50 (When measuring resistance under completely dry conditions)</li> <li>IP54 (When measuring current flowing through an insulated conductor, during storage)</li> <li>The protection rating for the enclosure of this instrument (based on EN60529) is IP20*, IP50*, or IP54*.</li> <li>* IP20, IP50, IP54:</li> <li>This indicates the degree of protection provided by the enclosure of the device for use in hazardous locations, entry of solid foreign objects, and the ingress of water.</li> <li>2: Protected against access to hazardous parts with a fingers. The equipment inside the enclosure is protected against entry by solid foreign objects larger than 12.5 mm in diameter.</li> <li>5: Protected against access to hazardous parts with wire measuring 1.0 mm in diameter. Dustproof type (The penetration of dust cannot be prevented completely, but quantities of dust that may hinder the stated operation of equipment or safety cannot penetrate the enclosure.)</li> <li>0: The equipment inside the enclosure is not protected against the harmful effects of water.</li> <li>4: The equipment inside the enclosure from any direction.</li> </ul>
Standards	Safety         EN 61010           EMC         EN 61326

Power supply	LR03 Alkaline batteries ×2 Rated supply voltage: 1.5 V DC × 2	
Continuous operating time	CM4371-50*1	About 40 hours (without the Z3210) About 20 hours (with the Z3210 installed and wirelessly communicating)
	CM4373-50*2	About 40 hours (without the Z3210) About 24 hours (with the Z3210 installed and wirelessly communicating)
	CM4375-50*2	About 40 hours (without the Z3210) About 20 hours (with the Z3210 installed and wirelessly communicating)
Dimensions*3	CM4371-50	Approx. 65W × 216H × 35D mm (2.56"W × 8.50"H × 1.38"D)
	CM4373-50	Approx. 65W × 250H × 35D mm (2.56"W × 9.84"H × 1.38"D)
	CM4375-50	Approx. 65W × 242H × 35D mm (2.56"W × 9.53"H × 1.38"D)
Jaw dimensions	CM4371-50	Approx. 69Wj × 14Dj mm (2.72"W × 0.55"D)
	CM4373-50	Approx. 92Wj × 18Dj mm (3.62"W × 0.71"D)
	CM4375-50	Approx. 53Wj × 20Dj mm (2.09"W × 0.79"D)
Jaw cross-sectional minimum dimension	CM4375-50	Approx. 9.5 mm (0.37")

#### **General Specifications**

Maximum	CM4371-50	φ33 mm
measurable conductor diameter	CM4373-50	φ55 mm
conductor diameter	CM4375-50	φ34 mm
Weight	CM4371-50	Approx. 340 g (12.0 oz., including batteries)
	CM4373-50	Approx. 530 g (18.7 oz., including batteries)
	CM4375-50	Approx. 350 g (12.3 oz., including batteries)
Product warranty duration	3 years or until the jaw open/close cycles reaches 30,000, whichever comes first	
Accessories	p.7	
Options	p.8	

<sup>\*1:</sup> Other prescribed conditions

When measuring 10 A AC, with the LCD not backlighted, values for reference purposes at 23°C

When measuring 100 A AC, with the LCD not backlighted, values for reference purposes at 23°C

<sup>\*2:</sup> Other prescribed conditions

<sup>\*3:</sup> The Jaw is not included in the dimensions of width and depth but in that of height.

# 3.2 Input Specifications, Measurement Specifications

#### (1) Basic specifications

Measurable range	See "3.3 Accuracy table" (p.75).	
Maximum rated voltage between terminals	1000 V AC (up to 1 kHz) 1000 V DC	
Maximum rated line-to- ground voltage	600 V (measurement category IV) 1000 V (measurement category III) Anticipated transient overvoltage: 8000 V	
Measurement method	True RMS measurement	
Measurement terminals	COM terminal, V terminal	

#### (2) Current measurement specifications

Maximum input current	As per the frequency derating characteristics (p.68)		
Coupling type	AC current*1	AC coupling	
	Other current measurement parameters	DC coupling	

## Input Specifications, Measurement Specifications

Display update rate*2	Auto A, AC current, DC current, AC+DC current		5 times/s		
	Current frequency		0.3 to 5.0 times/s (depending on the frequency)		
	DC power		1 time/s		
	DC current + DC voltage		2.5 times/s		
Zero-display range	Auto A, AC current, DC current, AC+DC current		5 counts or less		
Crest factor	Auto A, AC current, AC+DC current, inrush current				
	CM4371-50 20.00 /		range	7.5	
		600.0 A range		3 (500.0 A or less) 2.5 (more than 500.0 A but 600.0 A or less)	
	CM4373-50	600.0 A range		3 (500.0 A or less) 2.5 (more than 500.0 A but 600.0 A or less)	
	2000 A		range	2.84 (1000 A or less) 1.42 (more than 1000 A but 2000 A or less)	
	CM4375-50	1000 A range		1.5 (1000 A or less)	

Frequency detection input level	CM4371-50	20.00 A range	4.00 A or more*3		
		600.0 A range	20.0 A or more		
	CM4373-50	600.0 A range	40.0 A or more		
		2000 A range	200 A or more		
	CM4375-50	1000 A range	5.0 A or more*4		
Inrush trigger level	CM4371-50	20.00 A range	+2.0 A or more Otherwise, -2.0 A or less		
		600.0 A range	+10 A or more Otherwise, -10 A or less		
	CM4373-50	600.0 A range	+10 A or more Otherwise, -10 A or less		
		2000 A range	+100 A or more Otherwise, -100 A or less		
	CM4375-50	1000 A range	+10 A or more Otherwise, -10 A or less		
Peak detection time width	1 ms or more (with filter disabled)				

<sup>\*1:</sup> Does not apply to AC detection in Auto A mode.


<sup>\*2:</sup> Does not include range switching time.

<sup>\*3: 8.00</sup> A or more for 1 Hz  $\leq$  f  $\leq$  5 Hz

<sup>\*4: 10.0</sup> A or more for 1 Hz  $\leq$  f  $\leq$  5 Hz

# Frequency derating characteristics


CM4371-50



Inputting up to 1061 A of current is allowable for 1 minute or less. (66 Hz or less)

CM4373-50



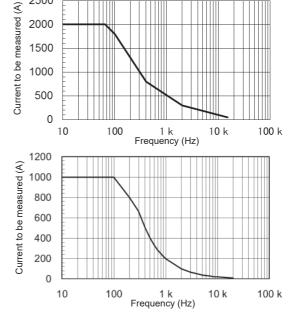

# Input Specifications, Measurement Specifications

# (3) Voltage measurement specifications

Overload protection	1100 V DC, 1100 V AC, or 2 × 10 <sup>7</sup> V·Hz, whichever is lower (Up to 1 minute of continuous application)		
Coupling type	AC voltage*1	AC coupling	
	Other voltage measurement parameters	DC coupling	
Input impedance	See "3.3 Accuracy table" (p.75	).	
Display update rate*2	Auto V, AC voltage, DC voltage, AC + DC voltage	5 times/s	
	Voltage frequency	0.3 to 5.0 times/s (depending on frequency)	
	DC power	1 time/s	
	DC current + DC voltage	2.5 times/s	
Zero-display range	Auto V, AC voltage, AC voltage + DC voltage	5 counts or less	
Crest factor	Auto V, AC voltage, AC voltage + DC voltage  6.000 V range, 60.00 V range, 600 3 (4000 counts or less) 2 (more than 4000 counts but 6000		
		1000 V range: 2 (750 counts or less) 1.5 (more than 750 counts but 1000 counts or less)	

Peak detection time width	1 ms or more (with filter disabled)	
Frequency detection input level	10% or more of each range's f.s.	
CMRR*3	AC voltage, AC+DC voltage 60 dB or more	
	DC voltage 100 dB or more	
NMRR*4	DC voltage 60 dB or more	

<sup>\*1:</sup> Does not apply to AC detection in Auto V mode.

<sup>\*2:</sup> Does not include range switching time.

<sup>\*3:</sup> Defined for 1 k $\Omega$  unbalance assuming that the input frequency is 0 Hz, 50 Hz, or 60 Hz.

<sup>\*4:</sup> Defined assuming that the input frequency is 50 Hz or 60 Hz.

# Input Specifications, Measurement Specifications

# (4) Other measurement parameters

	7		
Overload protection	1000 V DC, 1000 V AC, or 2 × 10 <sup>7</sup> V·Hz, whichever is lower (Up to 1 minute of continuous application)		
Overload current	At steady state: 30 mA or less At transient state: 1.5 A or less		
Display update rate*	Capacitance 0.5 to 5 times/s (depending on the capacitance)		
	Temperature (Type K thermocouple)	1 time/s (including thermocouple wiring break check)	
Response time	Continuity check  Open or short-circuit condition lasting for 0.5 ms of more can be detected.		
Open terminal voltage	Continuity check, resistance, diode 2.0 V DC or less		
Short-circuit detecting threshold	25 $\Omega$ ±10 $\Omega$ (continuous beep, LCD backlighted in red)		
Open-circuit detecting threshold	250 $\Omega$ ±10 $\Omega$		
Stabilization time for reference junction compensation of instrument	Up to 120 minutes (Reference: when the instrument having a temperature of 23°C is left to stand in ambient environments of 65°C for 60 minutes)		

<sup>\*:</sup> Does not include range switching time.

#### (5) DC High V Probe mode (in combination with the P2000)\*1

Maximum rated line-to- ground voltage	Conform to the specifications of the P2000.
Maximum rated voltage between terminals	Conform to the specifications of the P2000.
Overload protection	Conform to the specifications of the P2000.
Coupling type	DC coupling
Combinatorial measurement accuracy	<ul> <li>DC high voltage See "(11) DC high voltage (DC High V Probe mode)" (p.98) in "3.3 Accuracy table."</li> <li>DC power See "(18) DC power" (p.102) in "3.3 Accuracy table."</li> </ul>

<sup>\*1:</sup> The specifications above apply when both of the following two conditions are satisfied only: (1) the P2000 is connected, and (2) the instrument is in DC High V Prove mode.

# Input Specifications, Measurement Specifications

# (6) Accuracy specifications

Accuracy guarantee duration	1 year (duration for which accuracy shown in the accuracy table is guaranteed)     3 years (duration for which 1.5 times accuracy shown in the accuracy table is guaranteed), value for reference purposes	
Accuracy guarantee temperature and humidity range	23°C ±5°C (73°F ±9°F), 90% RH or less (non-condensing)	
Accuracy guarantee of current measurement, continuity check, and resistance measurement assumes that zero adjustment has been performed.  Temperature (Type K thermocouple) measurement requires use of the DT4910.		
Sine wave input		
See "3.3 Accuracy table" (p.75).		
CM4371-50 Within ±1.5%	rdg	
CM4373-50 Within ±1.0% rdg		
CM4375-50 Within ±1.5% rdg (for cables of $\phi$ 11 mm or more)		
Add [(measurement accuracy × 0.1)/°C] to measurement accuracy (outside the temperature range of 23°C ±5°C).		
	Accuracy guarantee temperature and humidity range  Accuracy guarantee of cur measurement assumes th Temperature (Type K there Sine wave input  See "3.3 Accuracy table" ( CM4371-50 Within ±1.5%  CM4373-50 Within ±1.5%  Add [(measurement accur.)]	

<sup>\*:</sup> At any position with respect to the jaw's center-point.

### (1) Auto A (AC/DC current automatic detection)

When AC is detected:

Conforms to the accuracy specifications described in "(4) AC+DC voltage" (p.82).

When DC is detected:

Conforms to the accuracy specifications described in "(3) DC current" (p.80).

## (2) AC current

#### Measured value/MAX/MIN/AVG (CM4371-50)

Range	Accuracy		Measurement accuracy	
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range	Filter disabled	Filter enabled
20.00 A	1.00 A to 20.00 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.10 A	±2.3% rdg ±0.10 A
(more	(0.01 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.08 A	±1.8% rdg ±0.08 A
than 2000 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±0.10 A	-
600.0 A	1.0 A to 600.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.5 A	±2.3% rdg ±0.5 A
(less than	(0.1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.3 A	±1.8% rdg ±0.3 A
180 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±0.5 A	_

### Measured value/MAX/MIN/AVG (CM4373-50)

Range	Accuracy		Measurement accuracy	
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range	Filter disabled	Filter enabled
600.0 A	1.0 A to 30.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±1.0 A	±2.3% rdg ±1.0 A
(more	(0.1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.8 A	±1.8% rdg ±0.8 A
than 6000		66 Hz < f < 1 kHz	±2.0% rdg ±1.0 A	-
counts)	30.1 A to 600.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.5 A	±2.3% rdg ±0.5 A
	(0.1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.3 A	±1.8% rdg ±0.3 A
		66 Hz < f < 1 kHz	±2.0% rdg ±0.5 A	-
2000 A	10 A to 1800 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±5 A	±2.3% rdg ±5 A
(less than	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±3 A	±1.8% rdg ±3 A
540 counts)	540 counts)	66 Hz < f < 1 kHz	±2.0% rdg ±5 A	-
	1801 A to 2000 A	10 Hz ≤ f < 45 Hz	±2.8% rdg ±5 A	±3.3% rdg ±5 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±2.3% rdg ±3 A	±2.8% rdg ±3 A
		66 Hz < f < 1 kHz	-	-

### Measured value/MAX/MIN/AVG (CM4375-50)

Accuracy		Accuracy guarantee	Measurement accuracy	
Range	guarantee range (resolution)	frequency range	Filter disabled	Filter enabled
1000 A	1.0 A to 30.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±1.0 A	±2.3% rdg ±1.0 A
	(0.1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.8 A	±1.8% rdg ±0.8 A
		66 Hz < f < 1 kHz	±2.0% rdg ±1.0 A	-
	30.1 A to 900.0 A (0.1 A)	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.5 A	±2.3% rdg ±0.5 A
		45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.3 A	±1.8% rdg ±0.3 A
		66 Hz < f < 1 kHz	±2.0% rdg ±0.5 A	-
	900.1 A to 999.9 A (0.1 A)	10 Hz ≤ f < 45 Hz	±2.3% rdg ±0.5 A	±2.8% rdg ±0.5 A
		45 Hz ≤ f ≤ 66 Hz	±1.8% rdg ±0.3 A	±2.3% rdg ±0.3 A
		66 Hz < f < 1 kHz	±2.5% rdg ±0.5 A	-

### PEAK MAX/ PEAK MIN (CM4371-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
20.00 A	±1.0 A to ±150.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 A
	(0.1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±0.7 A
600.0 A	±10 A to ±900 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±901 A to ±1500 A	10 Hz ≤ f < 45 Hz	±5.5% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±5.0% rdg ±7 A
		66 Hz < f < 1 kHz	±5.7% rdg ±7 A

### PEAK MAX/ PEAK MIN (CM4373-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
600.0 A	±10 A to ±1500 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
2000 A	±10 A to ±2300 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±2301 A to ±2840 A	10 Hz ≤ f < 45 Hz	±6.5% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±6.0% rdg ±7 A
		66 Hz < f < 1 kHz	-

### PEAK MAX/ PEAK MIN (CM4375-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
1000 A	±10 A to ±1000 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±1001 A to ±1500 A	10 Hz ≤ f < 45 Hz	±2.3% rdg ±7 A
	(1 A)	45 Hz ≤ f ≤ 66 Hz	±1.8% rdg ±7 A
		66 Hz < f < 1 kHz	±2.5% rdg ±7 A

### (3) DC current

### Measured value/MAX/MIN/AVG (CM4371-50)

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement accuracy
20.00 A	±1.00 A to ±20.00 A (0.01 A)	±1.3% rdg ±0.08 A
(more than 2000 counts)		
600.0 A	±1.0 A to ±600.0 A (0.1 A)	±1.3% rdg ±0.3 A
(less than 180 counts)		

#### Measured value/MAX/MIN/AVG (CM4373-50)

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement accuracy
600.0 A	±1.0 A to ±30.0 A (0.1 A)	±1.3% rdg ±0.8 A
(more than 6000 counts)	±30.1 A to ±600.0 A (0.1 A)	±1.3% rdg ±0.3 A
2000 A	±10 A to ±2000 A (1 A)	±1.3% rdg ±3 A
(less than 540 counts)		

#### Measured value/MAX/MIN/AVG (CM4375-50)

Rang	je	Accuracy guarantee range (resolution)	Measurement accuracy
1000 A		±1.0 A to ±30.0 A (0.1 A)	±1.3% rdg ±0.8 A
		±30.1 A to ±999.9 A (0.1 A)	±1.3% rdg ±0.3 A

### PEAK MAX/ PEAK MIN (CM4371-50)

Range	Accuracy guarantee range (resolution)	Measurement accuracy
20.00 A	±1.0 A to ±150.0 A (0.1 A)	±1.3% rdg ±0.7 A
600.0 A	±10 A to ±900 A (1 A)	±1.3% rdg ±7 A
	±901 A to ±1500 A (1 A)	±5.0% rdg ±7 A

#### PEAK MAX/ PEAK MIN (CM4373-50)

Range	Accuracy guarantee range (resolution)	Measurement accuracy
600.0 A	±10 A to ±1500 A (1 A)	±1.3% rdg ±7 A
2000 A	±10 A to ±2300 A (1 A)	±1.3% rdg ±7 A
	±2301 A to ±2840 A (1 A)	±6.0% rdg ±7 A

### PEAK MAX/ PEAK MIN (CM4375-50)

Range	Accuracy guarantee range (resolution)	Measurement accuracy
1000 A	±10 A to ±1000 A (1 A)	±1.3 % rdg ±7 A
	±1001 A to ±1500 A (1 A)	±1.8% rdg ±7 A

# (4) AC+DC voltage

# Measured value/MAX/MIN/AVG (CM4371-50)

Range	Accuracy		Measureme	nt accuracy
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range	Filter disabled	Filter enabled
20.00 A	1.00 A to 20.00 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.10 A	±2.3% rdg ±0.10 A
(more	(0.01 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.13 A	±1.8% rdg ±0.13 A
than 2000 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±0.10 A	-
600.0 A	1.0 A to 600.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 A	±2.3% rdg ±0.7 A
(less than	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±1.3 A	±1.8% rdg ±1.3 A
180 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±0.7 A	-

### Measured value/MAX/MIN/AVG (CM4373-50)

Range	Accuracy		Measureme	ent accuracy
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range	Filter disabled	Filter enabled
600.0 A	1.0 A to 30.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±1.2 A	±2.3% rdg ±1.2 A
(more than	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±1.8 A	±1.8% rdg ±1.8 A
6000 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±1.2 A	-
	30.1 A to 600.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 A	±2.3% rdg ±0.7 A
	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±1.3 A	±1.8% rdg ±1.3 A
		66 Hz < f < 1 kHz	±2.0% rdg ±0.7 A	-
2000 A	10 A to 1800 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A	±2.3% rdg ±7 A
(less than	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±13 A	±1.8% rdg ±13 A
540 counts)		66 Hz < f < 1 kHz	±2.0% rdg ±7 A	-
	1801 A to 2000 A	10 Hz ≤ f < 45 Hz	±2.8% rdg ±7 A	±3.3% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±2.3% rdg ±13 A	±2.8% rdg ±13 A
		66 Hz < f < 1 kHz	-	_

### Measured value/MAX/MIN/AVG (CM4375-50)

	Accuracy	Accuracy guarantee	Measurement accuracy	
Range	guarantee range (resolution)	frequency range	Filter disabled	Filter enabled
1000 A	1.0 A to 30.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±1.2 A	±2.3% rdg ±1.2 A
	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±1.8 A	±1.8% rdg ±1.8 A
		66 Hz < f ≤ 1 kHz	±2.0% rdg ±1.2 A	-
	30.1 A to 900.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 A	±2.3% rdg ±0.7 A
	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±1.3 A	±1.8% rdg ±1.3 A
		66 Hz < f ≤ 1 kHz	±2.0% rdg ±0.7 A	-
	900.1 A to 999.9 A	10 Hz ≤ f < 45 Hz	±2.3% rdg ±0.7 A	±2.8% rdg ±0.7 A
	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.8% rdg ±1.3 A	±2.3% rdg ±1.3 A
		66 Hz < f ≤ 1 kHz	±2.5% rdg ±0.7 A	_

### PEAK MAX/ PEAK MIN (CM4371-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
20.00 A	±1.0 A to ±150.0 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 A
	(0.1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±0.7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±0.7 A
600.0 A	±10 A to ±900 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±901 A to ±1500 A	10 Hz ≤ f < 45 Hz	±5.5% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±5.0% rdg ±7 A
		66 Hz < f < 1 kHz	±5.7% rdg ±7 A

### PEAK MAX/ PEAK MIN (CM4373-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
600.0 A	±10 A to ±1500 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
2000 A	±10 A to ±2300 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±2301 A to ±2840 A	10 Hz ≤ f < 45 Hz	±6.5% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±6.0% rdg ±7 A
		66 Hz < f < 1 kHz	-

### PEAK MAX/ PEAK MIN (CM4375-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
1000 A	±10 A to ±1000 A	10 Hz ≤ f < 45 Hz	±1.8% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.3% rdg ±7 A
		66 Hz < f < 1 kHz	±2.0% rdg ±7 A
	±1001 A to ±1500 A	10 Hz ≤ f < 45 Hz	±2.3% rdg ±7 A
	(1 A)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.8% rdg ±7 A
		66 Hz < f < 1 kHz	±2.5% rdg ±7 A

# (5) Current frequency, voltage frequency

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement accuracy
9.999 Hz	1.000 Hz to 9.999 Hz	±0.1% rdg ±0.003 Hz
(more than 9999 counts)	(0.001 Hz)	
99.99 Hz	1.00 Hz to 99.99 Hz	±0.1% rdg ±0.01 Hz
(more than 9999 counts, less than	(0.01 Hz)	
900 counts)		
999.9 Hz	1.0 Hz to 999.9 Hz	±0.1% rdg ±0.1 Hz
(less than 900 counts)	(0.1 Hz)	

# (6) Inrush current

### Measured inrush value (CM4371-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
20.00 A	3.00 A to 20.00 A (0.01 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±5.0% rdg ±0.13 A
600.0 A	10.0 A to 600.0 A (0.1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±5.0% rdg ±1.3 A

### Measured inrush value (CM4373-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
600.0 A	10.0 A to 600.0 A (0.1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±5.0% rdg ±1.3 A
2000 A	100 A to 1800 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±3.3% rdg ±13 A
	1801 A to 2000 A (1 A)	DC, 20 Hz ≤ f ≤ 66 Hz	±5.0% rdg ±13 A

### Measured inrush value (CM4375-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
1000 A	10.0 A to 999.9 A (0.1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±5.0% rdg ±1.3 A

### Inrush peak value (CM4371-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
20.00 A	±3.0 A to ±150.0 A (0.1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±6.0% rdg ±1.0 A
600.0 A	±10 A to ±900 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±6.0% rdg ±10 A
	±901 A to ±1500 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±9.7% rdg ±10 A

#### Inrush peak value (CM4373-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
600.0 A	±10 A to ±1500 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±6.0% rdg ±10 A
2000 A	±100 A to ±2300 A (10 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±6.0% rdg ±100 A
	±2310 A to ±2840 A (10 A)	DC, 20 Hz ≤ f ≤ 66 Hz	±8.0% rdg ±100 A

#### Inrush peak value (CM4375-50)

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range	Measurement accuracy
1000 A	±10 A to ±1000 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±6.0% rdg ±10 A
	±1001 A to ±1500 A (1 A)	DC, 20 Hz ≤ f ≤ 500 Hz	±8.0% rdg ±10 A

#### (7) Auto V (AC/DC voltage automatic detection)

When AC is detected: Conforms to the accuracy specifications described in "(10) AC+DC voltage" (p.95). When DC is detected: Conforms to the accuracy specifications described in "(9) DC voltage" (p.93).

#### (8) AC voltage

#### Measured value/MAX/MIN/AVG

Range	Accuracy		Measureme	nt accuracy	
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range*1 *2	Filter disabled	Filter enabled	Input impedance* <sup>3</sup>
6.000 V (more than	0.000 V to 0.299 V	15 Hz ≤ f < 45 Hz	±1.5% rdg ±0.015 V	±2.0% rdg ±0.015 V	3.2 MΩ ±5%
6000 counts) (0.001 V)	(0.001 V)	45 Hz ≤ f ≤ 66 Hz	±0.9% rdg ±0.013 V	±1.4% rdg ±0.013 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±0.015 V	-	
	0.300 V to 6.000 V	15 Hz ≤ f < 45 Hz	±1.5% rdg ±0.005 V	±2.0% rdg ±0.005 V	3.2 MΩ ±5%
	(0.001 V)	45 Hz ≤ f ≤ 66 Hz	±0.9% rdg ±0.003 V	±1.4% rdg ±0.003 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±0.005 V	-	

Range	Accuracy		Measureme	nt accuracy	
(automatic ranging threshold)	guarantee range (resolution)	Accuracy guarantee frequency range*1 *2	Filter disabled	Filter enabled	Input impedance* <sup>3</sup>
60.00 V (more than	3.00 V to 60.00 V	15 Hz ≤ f < 45 Hz	±1.5% rdg ±0.05 V	±2.0% rdg ±0.05 V	3.1 MΩ ±5%
6000 counts, less than 540	(0.01 V)	45 Hz ≤ f ≤ 66 Hz	±0.9% rdg ±0.03 V	±1.4% rdg ±0.03 V	
counts)	counts)	66 Hz < f < 1 kHz	±1.5% rdg ±0.05 V	-	
600.0 V (more than	30.0 V to 600.0 V (0.1 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg ±0.5 V	±2.0% rdg ±0.5 V	3.0 MΩ ±5%
6000 counts, less than 540		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg ±0.3 V	±1.4% rdg ±0.3 V	
counts)		66 Hz < f < 1 kHz	±1.5% rdg ±0.5 V	_	
1000 V (less than 540	50 V to 1000 V	15 Hz ≤ f < 45 Hz	±1.5% rdg ±5 V	±2.0% rdg ±5 V	3.0 MΩ ±5%
counts)	(1 V)	45 Hz ≤ f ≤ 66 Hz	±0.9% rdg ±3 V	±1.4% rdg ±3 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±5 V	-	

<sup>\*1:</sup> Accuracy within the frequency range of 15 Hz (inclusive) to 20 Hz (exclusive) is designed values.

<sup>\*2:</sup> Within the frequency range of less than 45 Hz, the accuracy guarantee assumes a superposed DC voltage of less than 500 V.

<sup>\*3:</sup> Defined assuming that the 50 Hz AC is input.

#### PEAK MAX/ PEAK MIN

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range*1 *2	Measurement accuracy
6.000 V	0 V to ±12.00 V	15 Hz ≤ f < 45 Hz	±1.8% rdg ±0.07 V
	(0.01 V)	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg ±0.07 V
		66 Hz < f < 1 kHz	±1.8% rdg ±0.07 V
60.00 V	±3.0 V to ±120.0 V	15 Hz ≤ f < 45 Hz	±1.8% rdg ±0.7 V
	(0.1 V)	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg ±0.7 V
		66 Hz < f < 1 kHz	±1.8% rdg ±0.7 V
600.0 V	±30 V to ±1000 V*3	15 Hz ≤ f < 45 Hz	±1.8% rdg ±7 V
	(1 V)	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg ±7 V
		66 Hz < f < 1 kHz	±1.8% rdg ±7 V
1000 V	±50 V to ±1000 V*4	15 Hz ≤ f < 45 Hz	±1.8% rdg ±7 V
	(1 V)	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg ±7 V
		66 Hz < f < 1 kHz	±1.8% rdg ±7 V

<sup>\*1:</sup> Accuracy within the frequency range of 15 Hz (inclusive) to 20 Hz (exclusive) is designed values.

<sup>\*2:</sup> Within the frequency range of less than 45 Hz, the accuracy guarantee assumes a superposed DC voltage of less than 500 V.

<sup>\*3:</sup> Values of up to ±1200 V are displayed, but accuracy is not defined for display values in excess of 1000 V (values for reference purposes).

<sup>\*4:</sup> Values of up to ±1500 V are displayed, but accuracy is not defined for display values in excess of 1000 V (values for reference purposes).

# (9) DC voltage

#### Measured value/MAX/MIN/AVG

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement accuracy	Input impedance (DC input)
600.0 mV	0.0 mV to ±600.0 mV	±0.5% rdg	6.7 MΩ ±5%
(more than 6000 counts)	(0.1 mV)	±0.5 mV	
6.000 V	0.000 V to ±6.000 V	±0.5% rdg	6.7 MΩ ±5%
(more than 6000 counts,	(0.001 V)	±0.003 V	
less than 540 counts)			
60.00 V	0.00 V to ±60.00 V	±0.5% rdg	6.1 MΩ ±5%
(more than 6000 counts,	(0.01 V)	±0.03 V	
less than 540 counts)			
600.0 V	0.0 V to ±600.0 V	±0.5% rdg	6.0 MΩ ±5%
(more than 6000 counts,	(0.1 V)	±0.3 V	
less than 540 counts)			
1000 V	0 V to ±1000 V	±0.5% rdg	6.0 MΩ ±5%
(less than 540 counts)	(1 V)	±3 V	

#### PEAK MAX/ PEAK MIN

Range	Accuracy guarantee range (resolution)	Measurement accuracy
600.0 mV	0 mV to ±1200 mV	±1.0% rdg ±7 mV
	(1 mV)	
6.000 V	0.00 V to ±12.00 V	±1.0% rdg ±0.07 V
	(0.01 V)	
60.00 V	0.0 V to ±120.0 V	±1.0% rdg ±0.7 V
	(0.1 V)	
600.0 V	0 V to ±1000 V	±1.0% rdg ±7 V
	(1 V)	
1000 V	0 V to ±1000 V	±1.0% rdg ±7 V
	(1 V)	

# (10) AC+DC voltage

#### Measured value/MAX/MIN/AVG

Range	Accuracy	Accuracy	Measurement accuracy		
(automatic ranging threshold)	guarantee range (resolution)	guarantee frequency range*1	Filter disabled	Filter enabled	Input impedance*2
6.000 V (more than 6000	0.000 V to 0.299 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.023 V	±2.0% rdg ±0.023 V	DC: 6.7 MΩ ±5% AC: 3.2 MΩ ±5%
counts)	(0.001 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.023 V	±1.5% rdg ±0.023 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±0.023 V	_	
	0.300 V to 6.000 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.013 V	±2.0% rdg ±0.013 V	DC: 6.7 MΩ ±5% AC: 3.2 MΩ ±5%
	(0.001 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.013 V	±1.5% rdg ±0.013 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±0.013 V	-	
60.00 V (more than	3.00 V to 60.00 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.13 V	±2.0% rdg ±0.13 V	DC: 6.1 MΩ ±5% AC: 3.1 MΩ ±5%
6000 counts, less than 540	(0.01 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.13 V	±1.5% rdg ±0.13 V	
counts)		66 Hz < f < 1 kHz	±1.5% rdg ±0.13 V	_	

Range	Accuracy	Accuracy Measurement accuracy			
(automatic ranging threshold)	guarantee range (resolution)	guarantee frequency range*1	Filter disabled	Filter enabled	Input impedance*2
600.0 V (more than	30.0 V to 600.0 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.7 V	±2.0% rdg ±0.7 V	DC: 6.0 MΩ ±5% AC: 3.0 MΩ ±5%
6000 counts, less than 540	(0.1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.7 V	±1.5% rdg ±0.7 V	
counts)		66 Hz < f < 1 kHz	±1.5% rdg ±0.7 V	_	
1000 V (less than 540	50 V to 1000 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±7 V	±2.0% rdg ±7 V	DC: 6.0 MΩ ±5% AC: 3.0 MΩ ±5%
counts)	(1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±7 V	±1.5% rdg ±7 V	
		66 Hz < f < 1 kHz	±1.5% rdg ±7 V	_	

<sup>\*1:</sup> Accuracy within the frequency range of 10 Hz (inclusive) to 20 Hz (exclusive) is designed values.

<sup>\*2:</sup> Defined assuming that the DC or 50 Hz AC is input.

#### PEAK MAX/ PEAK MIN

Range	Accuracy guarantee range (resolution)	Accuracy guarantee frequency range*1	Measurement accuracy
6.000 V	0.00 V to ±12.00 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.07 V
	(0.01 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.07 V
		66 Hz < f < 1 kHz	±1.5% rdg ±0.07 V
60.00 V	±3.0 V to ±120.0 V	10 Hz ≤ f < 45 Hz	±1.5% rdg ±0.7 V
	(0.1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±0.7 V
		66 Hz < f < 1 kHz	±1.5% rdg ±0.7 V
600.0 V	±30 V to ±1000 V*2	10 Hz ≤ f < 45 Hz	±1.5% rdg ±7 V
	(1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±7 V
		66 Hz < f < 1 kHz	±1.5% rdg ±7 V
1000 V	±50 V to ±1000 V*3	10 Hz ≤ f < 45 Hz	±1.5% rdg ±7 V
	(1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg ±7 V
		66 Hz < f < 1 kHz	±1.5% rdg ±7 V

<sup>\*1:</sup> Accuracy within the frequency range of 10 Hz (inclusive) to 20 Hz (exclusive) is designed values.

<sup>\*2:</sup> Values of up to ±1200 V are displayed, but accuracy is not defined for display values in excess of 1000 V (values for reference purposes).

<sup>\*3:</sup> Values of up to ±1500 V are displayed, but accuracy is not defined for display values in excess of 1000 V (values for reference purposes).

# (11) DC high voltage (DC High V Probe mode)

#### Measured value/MAX/MIN/AVG

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement accuracy (In combination with the P2000)	Input impedance (In combination with the P2000)
600.0 V	80.0 V to ±600.0 V	±1.0% rdg ±0.3 V	19.3 MΩ ±2%
(more than 6000 counts)	(0.1 V)		
2000 V	80 V to ±2000 V	±1.0% rdg ±3 V	19.3 MΩ ±2%
(less than 540 counts)	(1 V)		

# (12) Continuity check

Range	Accuracy guarantee range (resolution)	Measurement current	Measurement accuracy
600.0 Ω	0.0 Ω to 600.0 Ω (0.1 Ω)	200 μA ±20%	±0.7% rdg ±0.5 Ω

#### (13) Resistance

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Measurement current	Measurement accuracy
600.0 Ω	0.0 Ω to 600.0 Ω	200 μA ±20%	±0.7% rdg
(more than 6000 counts)	(0.1 Ω)		±0.5 Ω
6.000 kΩ	0.000 kΩ to 6.000 kΩ	100 μA ±20%	±0.7% rdg
(more than 6000 counts, less than 540 counts)	(0.001 kΩ)		±0.005 kΩ
60.00 kΩ	0.00 kΩ to 60.00 kΩ	10 μA ±20%	±0.7% rdg
(more than 6000 counts, less than 540 counts)	(0.01 kΩ)		±0.05 kΩ
600.0 kΩ	0.0 kΩ to 600.0 kΩ	1 μA ±20%	±0.7% rdg
(more than 6000 counts, less than 540 counts)	(0.1 kΩ)		±0.5 kΩ
6.000 MΩ	0.000 MΩ to 6.000 MΩ	100 nA ±20%	±1.0% rdg
(less than 540 counts)	(0.001 MΩ)		±0.005 MΩ

# (14) Diode

Range	Accuracy guarantee range (resolution)	Short-circuit current	Measurement accuracy
1.800 V	0.000 V to 1.800 V*1 (0.001 V)	200 μA ±20%	±0.7% rdg ±0.005 V

<sup>\*1:</sup> A series of beeps indicates forward connection (0.15 V to 1.8 V). A continuous beep is emitted and the LCD is backlighted in red if the voltage is less than 0.15 V.

#### (15) Capacitance

Range (automatic ranging threshold)	Accuracy guarantee range (resolution)	Charging current	Measurement accuracy
1.000 μF (more than 1100 counts)	0.000 μF to 1.100 μF (0.001 μF)	10 nA ±20% 100 nA ±20% 1 µA ±20%	±1.9% rdg ±0.005 μF
10.00 µF (more than 1100 counts, less than 100 counts)	0.00 μF to 11.00 μF (0.01 μF)	100 nA ±20% 1 µA ±20% 10 µA ±20%	±1.9% rdg ±0.05 µF
100.0 μF (more than 1100 counts, less than 100 counts)	0.0 μF to 110.0 μF (0.1 μF)	1 μA ±20% 10 μA ±20% 100 μA ±20%	±1.9% rdg ±0.5 µF
1000 μF (less than 100 counts)	0 μF to 1100 μF (1 μF)	10 μA ±20% 100 μA ±20% 200 μA ±20%	±1.9% rdg ±5 μF

## (16) Temperature (Type K thermocouple)

Thermocouple type	Unit	Accuracy guarantee range (resolution)	Measurement accuracy*1
K	°C	-40.0°C to 400.0°C (0.1°C)	±0.5% rdg ±3.0°C
K	°F*2	-40.0°F to 752.0°F (0.1°F)	±0.5% rdg ±5.4°F

<sup>\*1:</sup> Prescribed conditions (assuming that an ambient temperature where the instrument is left to stand stabilizes in the range of ±1°C)

<sup>\*2:</sup> The temperature unit can be switched over to Fahrenheit by a special operation on the instrument.

### (17) Electric charge detection (CM4371-50, CM4373-50)

Range	Detectable voltage range*1	Detectable frequency
High	Line-to-earth voltage: 40 V AC to 600 V AC	50 Hz/60 Hz
Low	Line-to-earth voltage: 80 V AC to 600 V AC	50 Hz/60 Hz

<sup>\*1:</sup> Prescribed condition

Assuming that the instrument is brought into contact with a 2 mm² 600 V polyvinyl chloride insulated wire or equivalent

# (18) DC power (CM4371-50)

Current range	Voltage range* <sup>1</sup> (input voltage range)	Accuracy guarantee range (resolution)	Measurement accuracy
20 A	600.0 mV (0.0 mV to ±600.0 mV)	0.00 VA to ±12.00 VA (0.01 VA)	±2.0% rdg ±0.20 VA
	6.000 V (±0.540 V to ±6.000 V)	0.0 VA to ±120.0 VA (0.1 VA)	±2.0% rdg ±2.0 VA
	60.00 V (±5.40 V to ±60.00 V)	0.000 kVA to ±1.200 kVA (0.001 kVA)	±2.0% rdg ±0.020 kVA
	600.0 V (±54.0 V to ±600.0 V)	0.00 kVA to ±12.00 kVA (0.01 kVA)	±2.0% rdg ±0.20 kVA
	1000 V (±540 V to ±1000 V)	0.00 kVA to ±20.00 kVA (0.01 kVA)	±2.0% rdg ±0.20 kVA
DC High V Probe mode	600.0 V (±80.0 V to ±600.0 V)	0.00 kVA to ±12.00 kVA* <sup>2</sup> (0.01 kVA)	±3.0% rdg ±0.20 kVA
	2000 V (±540 V to ±2000 V)	0.00 kVA to ±40.00 kVA (0.01 kVA)	±3.0% rdg ±0.20 kVA

Current range	Voltage range*1 (input voltage range)	Accuracy guarantee range (resolution)	Measurement accuracy
600 A	600.0 mV (0.0 mV to ±600.0 mV)	0.0 VA to ±360.0 VA (0.1 VA)	±2.0% rdg ±2.0 VA
	6.000 V (±0.540 V to ±6.000 V)	0.000 kVA to ±3.600 kVA (0.001 kVA)	±2.0% rdg ±0.020 kVA
	60.00 V (±5.40 V to ±60.00 V)	0.00 kVA to ±36.00 kVA (0.01 kVA)	±2.0% rdg ±0.20 kVA
	600.0 V (±54.0 V to ±600.0 V)	0.0 kVA to ±360.0 kVA (0.1 kVA)	±2.0% rdg ±2.0 kVA
	1000 V (±540 V to ±1000 V)	0 kVA to ±600 kVA (1 kVA)	±2.0% rdg ±20 kVA
DC High V Probe mode	600.0 V (±80.0 V to ±600.0 V)	0.00 kVA to ±360.0 kVA* <sup>2</sup> (0.1 kVA)	±3.0% rdg ±2.0 kVA
	2000 V (±540 V to ±2000 V)	0.00 kVA to ±1200 kVA (1 kVA)	±3.0% rdg ±20 kVA

#### Accuracy table

#### DC power (CM4373-50)

Current range	Voltage range* <sup>1</sup> (input voltage range)	Accuracy guarantee range (resolution)	Measurement accuracy
600 A	600.0 mV	0.0 VA to ±360.0 VA	±2.0% rdg ±2.0 VA
	(0.0 mV to ±600.0 mV)	(0.1 VA)	
	6.000 V	0.000 kVA to ±3.600 kVA	±2.0% rdg ±0.020 kVA
	(±0.540 V to ±6.000 V)	(0.001 kVA)	
	60.00 V	0.00 kVA to ±36.00 kVA	±2.0% rdg ±0.20 kVA
	(±5.40 V to ±60.00 V)	(0.01 kVA)	
	600.0 V	0.0 kVA to ±360.0 kVA	±2.0% rdg ±2.0 kVA
	(±54.0 V to ±600.0 V)	(0.1 kVA)	
	1000 V	0 kVA to ±600 kVA	±2.0% rdg ±20 kVA
	(±540 V to ±1000 V)	(1 kVA)	
DC High V	600.0 V	0.00 kVA to ±360.0 kVA*2	±3.0% rdg ±2.0 kVA
Probe mode	(±80.0 V to ±600.0 V)	(0.1 kVA)	
	2000 V	0.00 kVA to ±1200 kVA	±3.0% rdg ±20 kVA
	(±540 V to ±2000 V)	(1 kVA)	

Current range	Voltage range*1 (input voltage range)	Accuracy guarantee range (resolution)	Measurement accuracy
2000 A	600.0 mV (0.0 mV to ±600.0 mV)	0.000 kVA to ±1.200 kVA (0.001 kVA)	±2.0% rdg ±0.020 kVA
	6.000 V (±0.540 V to ±6.000 V)	0.00 kVA to ±12.00 kVA (0.01 kVA)	±2.0% rdg ±0.20 kVA
	60.00 V (±5.40 V to ±60.00 V)	0.0 kVA to ±120.0 kVA (0.1 kVA)	±2.0% rdg ±2.0 kVA
	600.0 V (±54.0 V to ±600.0 V)	0 kVA to ±1200 kVA (1 kVA)	±2.0% rdg ±20 kVA
	1000 V (±540 V to ±1000 V)	0 kVA to ±2000 kVA (1 kVA)	±2.0% rdg ±20 kVA
DC High V Probe mode	600.0 V (±80.0 V to ±600.0 V)	0.00 kVA to ±1200 kVA* <sup>2</sup> (1 kVA)	±3.0% rdg ±20 kVA
	2000 V (±540 V to ±2000 V)	0.00 kVA to ±4000 kVA (1 kVA)	±3.0% rdg ±20 kVA

#### Accuracy table

#### DC power (CM4375-50)

Current range	Voltage range*1 (input voltage range)	Accuracy guarantee range (resolution)	Measurement accuracy
1000 A	600.0 mV	0.000 kVA to ±0.600 kVA	±2.0% rdg ±0.020 kVA
	(0.0 mV to ±600.0 mV)	(0.001 kVA)	
	6.000 V	0.00 kVA to ±6.00 kVA	±2.0% rdg ±0.20 kVA
	(±0.540 V to ±6.000 V)	(0.01 kVA)	_
	60.00 V	0.0 kVA to ±60.0 kVA	±2.0% rdg ±2.0 kVA
	(±5.40 V to ±60.00 V)	(0.1 kVA)	
	600.0 V	0 kVA to ±600 kVA	±2.0% rdg ±20 kVA
	(±54.0 V to ±600.0 V)	(1 kVA)	
	1000 V	0 kVA to ±1000 kVA	±2.0% rdg ±20 kVA
	(±540 V to ±1000 V)	(1 kVA)	
DC High V	600.0 V	0 kVA to ±600 kVA*2	±3.0% rdg ±20 kVA
Probe mode	(±80.0 V to ±600.0 V)	(1 kVA)	
	2000 V	0 kVA to ±2000 kVA	±3.0% rdg ±20 kVA
	(±540 V to ±2000 V)	(10 kVA)	

<sup>\*1:</sup> DC power ranges will be automatically switched in sync with the voltage range.

<sup>\*2:</sup> When a voltage of less than 80.0 V is input, the LCD shows [- - - -kVA].



## **Maintenance and Service**

## 4.1 Troubleshooting

Problem	Cause	Remedy		
The instrument is indicating an abnormal measured value.	The measured value is lower than the lower limit value of the measuring range.	Wrap the wire around the jaw one or more times. Wrapping the wire $n$ times can increase the displayed value by $(n + 1)$ times.		
	The tips of the jaw open.	Close the jaw tips.		
	The jaw is damaged.	The instrument with its jaw damaged cannot measure current accurately. Have the instrument repaired.		
	Displayed values can frequently fluinput. This, however, is not a malfu	uctuate due to induction potential even with no unction.		
Measured value differ from those of another clamp-on current meter.	Measured waveforms contain a component that falls outside the frequency characteristics range.	The instrument cannot accurately measure waveforms that contain a component that falls outside the frequency characteristics range.		
	The instrument, which uses the true RMS method, can accurately measure distorted waveforms. When measuring a distorted waveform, the measure will differ from a clamp-on current meter that uses the averaging method.			

#### Troubleshooting

Problem	Cause	Remedy
The current value is larger than expected. A current value is displayed even with no input.	There is a transformer or high- current circuit that emits a strong magnetic field near the instrument. Otherwise, there is a wireless device that emits a strong electric field.	Perform measurement keeping the instrument away from such equipment.
The instrument's jaw emits sound (vibration).	Greater than or equal to 500 A of AC current is being measured.	The jaw may emit sound (vibration); however, there is no effect on the measurement.
The measured value does not appear.	The test leads have a break.	Check the continuity of the test leads. (p.43) If a break is found, replace the test leads.
No measured value is displayed even when the test lead tips are shorted.	The test leads are not inserted all the way.	Insert the test leads all the way.
Zero adjustment is impossible.	Zero adjustment was performed leaving the instrument clamped around a measurement target.	If you wish to measure current, remove the instrument from a measurement target to perform zero adjustment.

If problems cannot be resolved even after you have implemented such remedies, have the instrument repaired.

## 4.2 Error and Operation Displays

Error display	Description	Remedy
v.UP	The instrument's firmware is being upgraded.	Do not remove the batteries until the upgrade completes.
Err 001	ROM error (program)	
Err 002	ROM error (adjustment data)	When the error appears on the display, it is necessary to repair the instrument. Please
Err 004	Memory error	contact your authorized Hioki distributor or
Err 005	ADC error (hardware malfunction)	reseller.
Err 008	Z3210 communication error (the Z3210 is malfunctioning or is not properly connected)	Perform the following steps. (p.25) Disconnect and then reconnect the Z3210. If you have another Z3210, replace the unit in question with that one. If the error continues to be displayed, the instrument needs to be repaired. Please contact your authorized Hioki distributor or reseller.

## 4.3 Cleaning

#### **ACAUTION**



If the instrument becomes dirty, wipe the instrument clean with a soft cloth moistened with water or a neutral detergent.

Never use solvents such as benzene, alcohol, acetone, ether, ketone, thinners or gasoline. Doing so could deform and discolor the instrument.

#### **IMPORTANT**

■ Keep the facing core surfaces of the jaws clean by gently wiping them with a soft dry cloth.

Dirt on the facing core surfaces of the jaws can adversely affect the measurement accuracy.

Wipe the LCD gently with a soft, dry cloth.

## **Appendix**

### 5.1 Voltage Detection Function

Check the instrument for proper operation by measuring a power supply with a known voltage, such as a commercial power supply, before use.

The voltage detection function cannot operate correctly for the following circuits and wires:


- Non-grounded circuits, of which the line-to-earth voltage is not fixed, such as the secondary side of transformers
- · DC circuits
- · Grounded wires
- · Shielded wires


It is recommended that you set the voltage detection function to High. If the voltage detection function malfunctions due to the effect of a nearby wire, set the sensitivity to Low. However, depending on the use environment, the instrument with the sensitivity set to Low may not be able to detect even a voltage within the detection range.

#### Measurement principle

The instrument employs a voltage-detecting method using electrostatic coupling to determine the live condition of objects under test.

See"(17) Electric charge detection (CM4371-50, CM4373-50)" (p. 101) for information about the detectable voltage range and detectable frequency.





Equivalent circuit diagram

Although a detected current will flow to the ground through your body, the current, less than 1  $\mu$ A, will not adversely affect you.

#### **IMPORTANT**


If it is difficult to judge with the voltage detection function, check the voltage using the voltage measuring function.

## 5.2 Example of Use

#### Checking for noise superimposed on DC voltage and current

Measure voltage/current values and voltage/current peak values of each DC component, AC component, and AC+DC resultant component.

Example: A DC voltage of 100 V with an AC voltage of 10 V superimposed

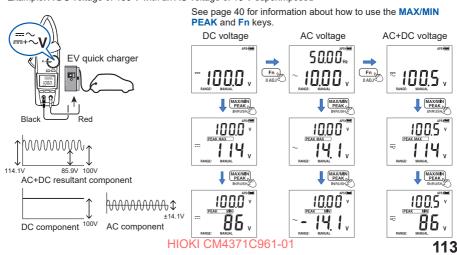

Example of Use

## Index

Α	D
AC+DC current       36         AC+DC voltage       37, 95         AC current       36, 75         AC voltage       37, 90         Automatic hold       34, 35         Automatic power save       46, 59         Average       40	DC current       36, 45         DC High V Probe mode       47         DC power       45         DC voltage       37, 45, 59, 93         Degrees Fahrenheit       60         Diode       37, 43, 99         Displayed value fluctuation       107         DT4910 Thermocouples (K)       44
Backlight       24, 46, 59         Flashing       42         Illuminate in red       33, 43         Buzzer       24, 33, 42, 59	Error and Operation Display
C	F
Capacitance	Filter

G	N
GENNECT Cross 51	Noise
н	Р
HID 55	Peak value
Inrush current 41, 87	
Jaws	Range
L	Serial number
L9300	Switching the temperature units 60
М	T
Manual hold	Temperature

Voltage	42,	70
---------	-----	----

#### V

Wire break	5,	21,	44,	108
Wireless Adapter			. 22	, 51
Wireless communications functi	on			. 51

#### Z

Z3210			. 22	, 51
Zero adjustment	32,	41,	43,	108

Index



Model	Serial number	Warranty period Three (3) years from date of purchase (/)
Customer name:		
Customer address:		
Important		
· Please retain this warran	. Please retain this warranty certificate Dunicates cannot be reissued	-

address. The personal information you provide on this form will only be used to provide repair service and information · Complete the certificate with the model number, serial number, and date of purchase, along with your name and about Hioki products and services

Please contact the place of purchase in the event of a malfunction and provide this document, in which case Hioki will This document certifies that the product has been inspected and verified to conform to Hioki's standards. repair or replace the product subject to the warranty terms described below.

# Warranty terms

- If the date of purchase is unknown, the warranty period is defined as three (3) years from the date (month and year) of manufacture (as indicated by the first four digits of the serial number in YYMM format). 1. The product is guaranteed to operate properly during the warranty period (three [3] years from the date of purchase).
  - The accuracy of measured values and other data generated by the product is guaranteed as described in the product 2. If the product came with an AC adapter, the adapter is warrantied for one (1) year from the date of purchase.
    - 4. In the event that the product or AC adapter malfunctions during its respective warranty period due to a defect of
- The following malfunctions and issues are not covered by the warranty and as such are not subject to free repair or workmanship or materials, Hioki will repair or replace the product or AC adapter free of charge.
- -1. Malfunctions or damage of consumables, parts with a defined service life, etc. Malfunctions or damage of connectors, cables, etc.

HIOKI CM4371C961-01

- Malfunctions or damage caused by shipment, dropping, relocation, etc., after purchase of the product
   Malfunctions or damage caused by inappropriate handling that violates information found in the instruction manual or
  - Malfunctions or damage caused by a failure to perform maintenance or inspections as required by law or on precautionary labeling on the product itself
- -6. Malfunctions or damage caused by fire, storms or flooding, earthquakes, lightning, power anomalies recommended in the instruction manual
  - Damage that is limited to the product's appearance (cosmetic blemishes, deformation of enclosure shape. (involving voltage, frequency, etc.), war or unrest, contamination with radiation, or other acts of God fading of color, etc.)
- Other malfunctions or damage for which Hioki is not responsible
- The warranty will be considered invalidated in the following circumstances, in which case Hioki will be unable to perform service such as repair or calibration:
  - -2. If the product has been embedded in another piece of equipment for use in a special application (aerospace -1. If the product has been repaired or modified by a company, entity, or individual other than Hioki
- 7. If you experience a loss caused by use of the product and Hioki determines that it is responsible for the underlying issue nuclear power, medical use, vehicle control, etc.) without Hioki's having received prior notice
- -1. Secondary damage arising from damage to a measured device or component that was caused by use of the product Hioki wi provide compensation in an amount not to exceed the purchase price, with the following exceptions:
  - Damage arising from measurement results provided by the product N
    - -3 Damage to a device other than the product that was sustained when connecting the device to the product (including via network connections)
- of time has passed since their manufacture, products whose parts have been discontinued, and products that cannot be 8 Hioki reserves the right to decline to perform repair, calibration, or other service for products for which a certain amount HIOKI E.E. CORPORATION repaired due to unforeseen circumstances.

http://www.hioki.com

18-07 EN-3

## HIOKI





All regional contact information

#### **HEADQUARTERS**

81 Koizumi Ueda, Nagano 386-1192 Japan

#### **HIOKI EUROPE GmbH**

Helfmann-Park 2 65760 Eschborn, Germany hioki@hioki.eu

2111 FN

Edited and published by HIOKI E.E. CORPORATION

Printed in Japan

- CE declarations of conformity can be downloaded from our website.
- ·Contents subject to change without notice.
- This document contains copyrighted content.
- •It is prohibited to copy, reproduce, or modify the content of this document without permission.
- Company names, product names, etc. mentioned in this document are trademarks or registered trademarks of their respective companies.